

AC AUTOMATIC INSULATION/ WITHSTANDING HiTESTER 3174

Safety Standards Measuring Instruments



Featuring contact check functionality

The effects of test lead wire breaks, erroneous test results caused by faulty contact, and fluctuations in test voltage caused by variations in the instrument's supply voltage on withstanding voltage and insulation resistance testing are well known.

The AC Automatic Insulation/Withstanding HiTester 3174 is a **low-cost solution featuring contact check functionality as well as a stabilized power supply** to prevent the reduced test reliability that can result from these issues.

To streamline production line test processes, the HiTester also features configuration of test parameters via RS-232C (GP-IB) and reading of parameters from the EXT I/O interface.


Improved Test Reliability

NEW

● Contact check function improves test reliability


The 3174's contact check function lets you **detect test lead wire breaks and faulty contact** during testing by sensing measurement issues in real time.

◆ If a test lead wire were to break during testing with a tester that does not offer contact check functionality, defective test pieces would be judged to be non-defective.

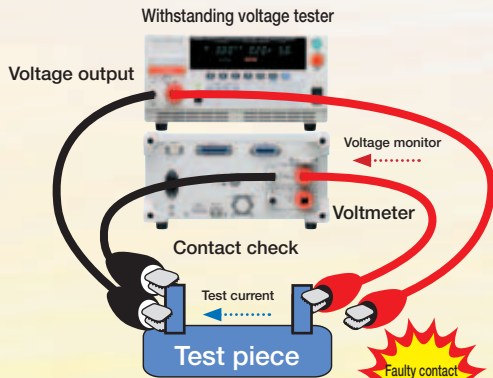

The 3174 improves test reliability by monitoring voltage to detect lose leads during testing and faulty wiring during measurement.

*Since contact check is performed while testing is in progress, use of contact check functionality does not increase cycle time.

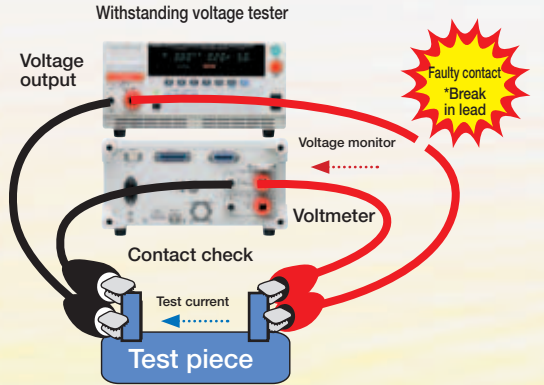

◆ If a test lead were to come lose during testing with a measurement device that does not offer contact check functionality, defective test pieces would be judged to be non-defective.

Fluorescent display tube
The display uses a bright, easy-to-read fluorescent tube.

DANGER lamp

Flashes a warning during testing and whenever high voltage is present at the terminals.
The DANGER lamp turns off when the voltage at the output terminals is no greater than AC 30 V or DC 60 V.



9613
SINGLE-HAND
REMOTE CONTROL
(option)

9614
TWO-HAND
REMOTE CONTROL
(option)

External switch

Enables start/stop control by means of the 9613 SINGLE-HAND REMOTE CONTROL or 9614 TWO-HAND REMOTE CONTROL.
(The 9613 and 9614 are optional.)

Test mode selection

Select from three test modes:
1. Manual test mode: W (withstand voltage testing) / I (insulation resistance testing)
2. Automatic test mode: W→I / I→W



NEW

● Judgment output at forced stop

The ability to obtain a judgment even after a forced stop increases testing freedom.

NEW

● Continued analytical testing after FAIL judgments

Test pieces can now be analyzed by means of detailed monitoring of the test current accompanying FAIL judgments.

● Ramp timer function

The ramp-up initial value, ramp-up and ramp-down time parameters can be set independently.

● True effective value display

● Eliminate the effects of supply voltage fluctuations

● Delay timer function

Safe, Automated Operation

Convenient


- Continuous full-auto withstanding voltage and insulation resistance testing

The 3174 lets you **set independent test conditions including test voltage for withstanding voltage and insulation resistance testing**, and you can perform these tests continuously. Press the W→I key to automatically perform withstanding voltage followed by insulation resistance tests, or press the I→W key to automatically perform insulation resistance followed by withstanding voltage tests.

Safe

- Interlock function

Signal input from an external device such as an automatic tester can be used to disable output and prevent testing, **ensuring safety during automatic testing and other uses.**

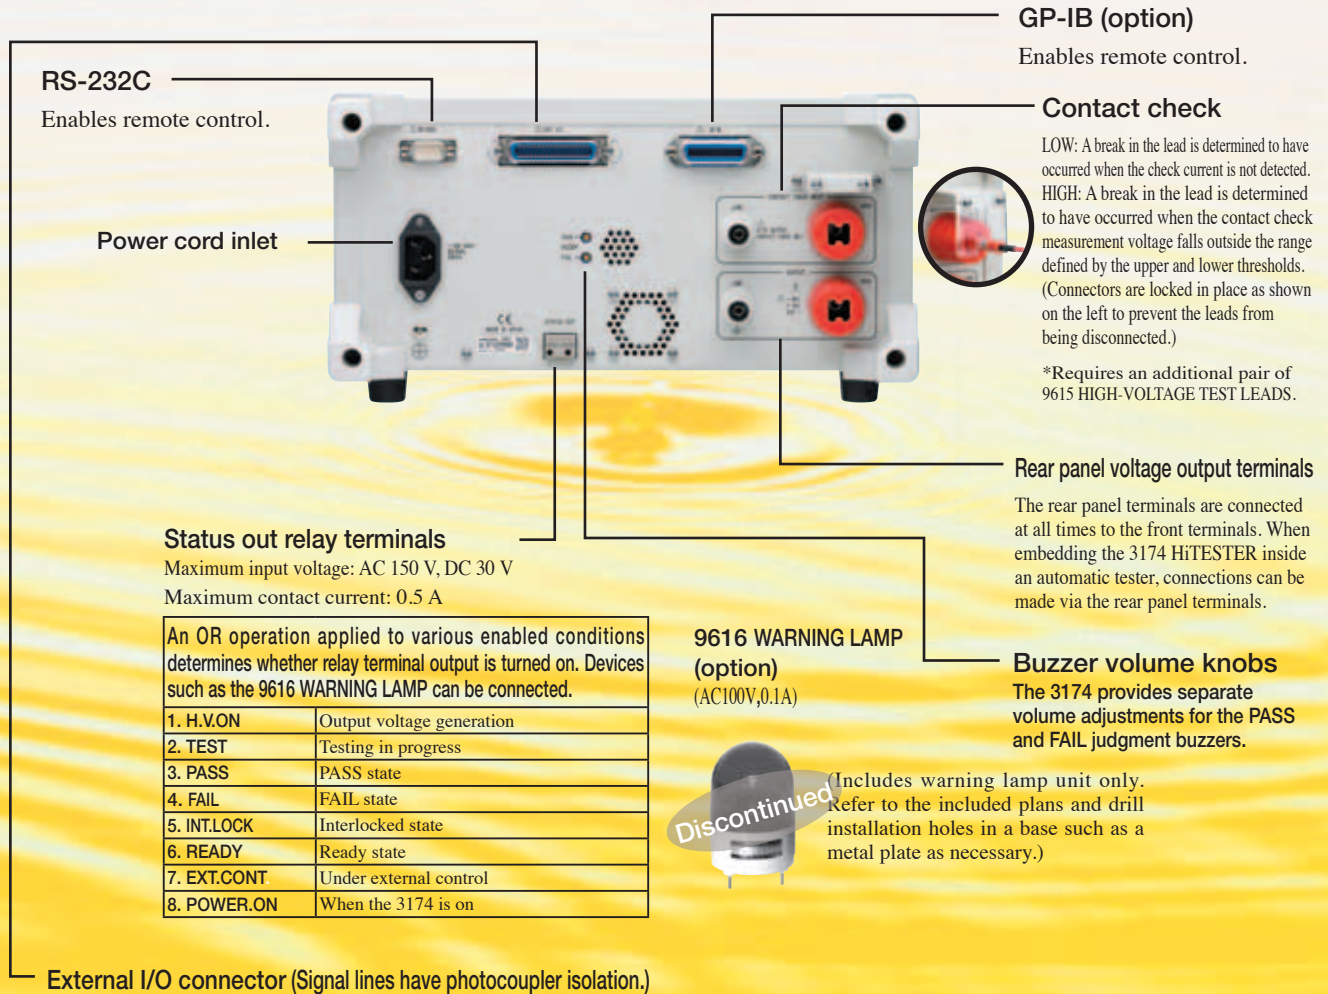

RS-232C
Enables remote control.

Power cord inlet

GP-IB (option)
Enables remote control.

Contact check
LOW: A break in the lead is determined to have occurred when the check current is not detected.
HIGH: A break in the lead is determined to have occurred when the contact check measurement voltage falls outside the range defined by the upper and lower thresholds. (Connectors are locked in place as shown on the left to prevent the leads from being disconnected.)
*Requires an additional pair of 9615 HIGH-VOLTAGE TEST LEADS.

Rear panel voltage output terminals
The rear panel terminals are connected at all times to the front terminals. When embedding the 3174 HiTESTER inside an automatic tester, connections can be made via the rear panel terminals.

Status out relay terminals
Maximum input voltage: AC 150 V, DC 30 V
Maximum contact current: 0.5 A

An OR operation applied to various enabled conditions determines whether relay terminal output is turned on. Devices such as the 9616 WARNING LAMP can be connected.

1. H.V.ON	Output voltage generation
2. TEST	Testing in progress
3. PASS	PASS state
4. FAIL	FAIL state
5. INT.LOCK	Interlocked state
6. READY	Ready state
7. EXT.CONT.	Under external control
8. POWER.ON	When the 3174 is on

9616 WARNING LAMP (option)
(AC100V,0.1A)

Buzzer volume knobs
The 3174 provides separate volume adjustments for the PASS and FAIL judgment buzzers.

External I/O connector (Signal lines have photocoupler isolation.)

Pin	I/O	Signa	Function
1	OUT	READY	Low in ready state
2	OUT	L-FAIL	Low in FAIL state (lower bound)
3	OUT	U-FAIL	Low in FAIL state (upper bound)
4	OUT	PASS	Low in PASS state
5	OUT	TEST	Low in test state
6	OUT	H.V.ON	Low when voltage is present at output terminals
7	IN	EXT-E	When low, external I/O input signals are enabled
8	IN	START	When low, same function as START key
9	IN	STOP	When low, same function as STOP key
10	IN	INT.LOCK	Interlock on open
11	OUT	W-MODE	Low during withstanding voltage testing
12	OUT	I-MODE	Low during insulation resistance testing
13	OUT	W-FAIL	Low in FAIL state during withstand voltage testing
14	OUT	I-FAIL	Low in FAIL state during insulation resistance testing
15-18	IN	ISO.COM	Ground inputs for external devices
22-25	IN	MEM-0 to 3	Saved test selected pins
27	IN	MEM-E	When low, enables memory selected pins
28-29	OUT	MODE-0,1	Current test mode
33-36	OUT	ISO.DCV	Internal DC 15 V power supply (100 mA)

Interface specifications

EXT I/O : Output signals

Open collector output (with photocoupler isolation)
All active low with a maximum load voltage of DC 30 V
Maximum output current: DC 100 mA per signal
Output saturation voltage: DC 1.5 V or less

Input signals

All active low input (with photocoupler isolation)
Maximum applied voltage: 30 V
High level voltage: from DC 15 V to 30 V, or open
Low level voltage: DC 5 V or less (-6 mA typ.)

EXT SW : Input signals (contact input)

START, STOP, SW.EN (external switch terminal enable)

Output signals

LED activation signal (maximum load current: 40 mA)

AC AUTOMATIC INSULATION/WITHSTANDING HITESTER 3174

Withstanding Voltage Testing

Test Voltage

Output voltage	: AC 0.2 to 5 kV (50/60 Hz), single-range output
Voltage output method	: PWM switching method (0 V start; voltage can be changed while generating output)
Voltage specification method	: Digital (setting resolution: 0.01 kV)
Output voltage accuracy	: $\pm 1.5\%$ of setting ± 20 V
Maximum rated output	: AC 100 VA (5 kV/20 mA) continuous rating
Transformer capacity	: 100VA
Voltmeter	: True effective value display Digital meter: AC 0 kV to 5.00 kV Accuracy: $\pm 1.5\%$ rdg (1,000 V or less, ± 15 V)
Output waveform	: Sine wave
Voltage change rate	: 15% or less (converges to setting within 1 s during change from maximum rated load to no load)
Distortion factor	: 5% or less (tester impedance during measurement with 5 kV output under 40 M Ω load)
Frequency	: 50/60Hz ($\pm 0.2\%$)

Current Detection

Current measurement range	: 0.01 mA to 20 mA (2 ranges)
Measurement range	: 10mA/20mA
Indicated value	: True effective value display
Measurement ranges and resolutions	: 0.00 mA to 10.00 mA, 0.01 mA (10 mA range) 0.0 mA to 20.0 mA, 0.1 mA (20 mA range)
Measurement accuracy	: $\pm 2\%$ rdg ± 0.05 mA (10 mA range) $\pm 2\%$ rdg ± 0.5 mA (20 mA range)

Insulation Resistance Measurement

Test Voltage

Rated voltage	: DC 500 V/1,000 V (positive polarity)
Unloaded voltage	: 1 to 1.2 times rated voltage
Rated measurement current	: 1 to 1.2 mA
Short-circuit current	: 4 to 5 mA (500 V), 2 to 3 mA (1,000 V)
Measurement range	: 0.2 to 2,000 M Ω (500 V), 0.5 to 2,000 M Ω (1,000 V)
Guaranteed accuracy ranges/accuracies	: 0.5 to 999 M Ω (500 V), 1 M Ω to 999 M Ω (1,000 V): $\pm 4\%$ rdg 1,000 M Ω to 2,000 M Ω : $\pm 8\%$ rdg
Measurement resolution	: 0.01 M Ω (0.20 M Ω to 19.9 M Ω) 0.1 M Ω (20.0 M Ω to 199.9 M Ω), 1 M Ω (200 M Ω to 2,000 M Ω)
Measured resistance ranges	: 2 M Ω , 20 M Ω , 200 M Ω , 2,000 M Ω (500 V) 4 M Ω , 40 M Ω , 400 M Ω , 2,000 M Ω (1,000 V)

Timers

Setting range	: 0.3 to 999 s
Operation	: When set to on: Display counts down from the set time after start. When set to off: Display indicates time elapsed since start.
Setting resolution/accuracy	: 0.1 s (0.3 to 99.9 s) ± 50 ms 1 s (100 to 999 s) ± 0.5 s

Ramp Timers (Withstand voltage testing)

Setting range	: 0.1 to 99.9 s: Ramp-up and ramp-down can be set independently.
Operation	: Ramp-up: The output voltage increases linearly from the initial voltage to the test voltage over the ramp-up time. Ramp-down: The output voltage decreases from the set voltage to 0 V over the ramp-down time after the test time elapses, and the display counts down from the set time. *The actual ramp-up waveform varies with the load due to the analog response delay.

Setting resolution	: 0.1s
--------------------	--------

Delay Timers (Insulation resistance testing)

Setting range	: 0.1 to 99.9 s
Setting resolution	: 0.1s

Decision Function

Decision method	: Window comparison method with upper and lower bound settings (digital specification)
Decision results	: UPPER-FAIL: The measured current (measured insulation value) exceeded the specified upper threshold. PASS: The measured current (measured insulation value) fell within the range defined by the specified upper and lower thresholds. LOWER-FAIL: The measured current (measured insulation value) was less than the specified lower bound. UPPER LOWER-FAIL: A testing error occurred, for example due to a failure to generate the set voltage.
Decision processing	: Display, buzzer, and EXT I/O signal output is generated according to each decision result.
Setting range	: AC withstanding voltage: 0.1 to 20.0 mA (upper threshold), 0.1 to 19.9 mA (lower threshold) DC insulation: 0.2 to 2,000 M Ω (500 V) or 1.0 to 2,000 M Ω (1,000 V) for both upper and lower thresholds
Setting resolution	: AC withstanding voltage: 0.1 mA DC insulation: 0.01 M Ω (0.2 to 2.00 M Ω), 0.1 M Ω (2.10 to 20.0 M Ω), 1 M Ω (21.0 to 200 M Ω), 10 M Ω (210 to 2,000 M Ω)

Contact Check

Voltmeter accuracy	: Detection method: Average value detection/effective value conversion Accuracy: Setting ± 50 V *Inaccuracy may increase when the waveform is distorted.
Decision results	: Enables the contact check function (does not increase cycle time). LOW: A break in the lead is determined to have occurred when the check current is not detected. HIGH: Upper and lower thresholds for the check detection voltage can be set. A break in the lead is determined to have occurred when the contact check measurement voltage falls outside the range defined by the upper and lower thresholds.
Voltage setting range	: Withstanding voltage testing: 0.20 kV to 5.0 kV (0.01 kV resolution; applies to both upper and lower thresholds) Insulation resistance measurement: Upper threshold of 600 V and lower threshold of 500 V (during 500 V measurement); upper threshold of 1,200 V and lower threshold of 1,000 V (during 1,000 V measurement) (both fixed)

General Specifications

Display	: Fluorescent display tube (digital display)
Monitor functions	: Output voltage, detected current, insulation resistance
Monitor period	: 2 times per second, minimum
Operating temperature range	: 0°C to 40°C, 80% RH or less (non-condensing)
Storage temperature range	: -10°C to 50°C, 90% RH or less (non-condensing)
Temperature and humidity range for guaranteed accuracy	: 23 ± 5 °C, 80% RH or less (non-condensing) (With warm-up period of at least 10 min)
Guaranteed accuracy term	: 1 year
Operating environment	: Indoors at elevations of up to 2,000 m at a pollution level of 2
Supply voltage	: AC 100 to 240 V Designed to tolerate voltage fluctuations of $\pm 10\%$ of the rated supply voltage.
Power supply frequency	: 50Hz/60Hz
Withstanding voltage	: Power supply to chassis: 1.39 kV at 10 mA for 15 s
Maximum rated power	: 200VA
Dimensions	: Approx. 320 (W) x 155 (H) x 395 (D) mm (excluding protruding parts)
Weight	: Approx. 15 kg
Applicable standards	: EMC: EN61326 Class A, EN61000-3-2, EN61000-3-3, Safety: EN61010-1
Included accessories	: HIGH-VOLTAGE TEST LEADS 9615 (1 each high-voltage and return), power cord, disconnection prevention plate

Model

AC AUTOMATIC INSULATION/WITHSTANDING HITESTER 3174
AC AUTOMATIC INSULATION/WITHSTANDING HITESTER 3174-01 (GP-IB Model)

Options

ELECTRIC SAFETY TESTING SOFTWARE	9267
SINGLE-HAND REMOTE CONTROL	9613
TWO-HAND REMOTE CONTROL	9614
HIGH-VOLTAGE TEST LEADS	9615
RS-232C CABLE (9-pin to 9-pin/cross/1.8 m)	9637
RS-232C CABLE (9-pin to 25-pin/cross/1.8 m)	9638
GP-IB CONNECTING CABLE (2 m)	9151-02

Note: Company names and Product names appearing in this catalog are trademarks or registered trademarks of various companies.

HIOKI

HIOKI E. E. CORPORATION

HEADQUARTERS

81 Koizumi, Ueda, Nagano, 386-1192, Japan
TEL +81-268-28-0562 FAX +81-268-28-0568
http://www.hioki.com / E-mail: os-com@hioki.co.jp

HIOKI USA CORPORATION

TEL +1-609-409-9109 FAX +1-609-409-9108
http://www.hiokiusa.com / E-mail: hioki@hiokiusa.com

HIOKI (Shanghai) SALES & TRADING CO., LTD.
TEL +86-21-63910090 FAX +86-21-63910360
http://www.hioki.cn / E-mail: info@hioki.com.cn

HIOKI INDIA PRIVATE LIMITED
TEL +91-124-6590210 FAX +91-124-6460113
E-mail: hioki@hioki.in

HIOKI SINGAPORE PTE. LTD.
TEL +65-6634-7677 FAX +65-6634-7477
E-mail: info-sg@hioki.com.sg

HIOKI KOREA CO., LTD.
TEL +82-42-936-1281 FAX +82-42-936-1284
E-mail: info-kr@hioki.co.jp

DISTRIBUTED BY